

Clearing VistaView Application Cache


Please follow the steps below to clear the application's cache for better performance. This will **not** remove any patient data stored on the device.

1. Start by unplugging the device and navigating to the home screen by pressing the home button.
2. Press the task button and clear the VistaView application by swiping up on the window




Task Button

3. Press and hold the VistaView app icon until you see an option appear called **App Info**. Select that option.

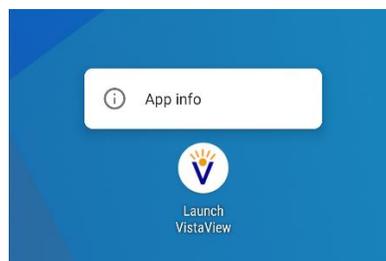




4. Select **Storage** → Select **Clear Cache** → Select **Ok**. The “Clear Cache” button should be grayed out.

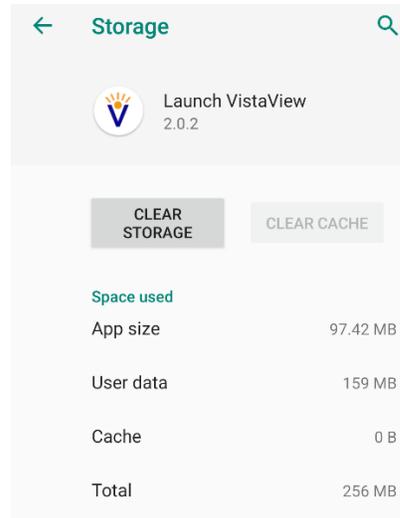

5. Go back to the main menu by pressing the home button and open the VistaView application.
6. In the application main menu, go to **Settings** in the upper-right corner → Select **Bluetooth** → then select **Seek Devices**. Fundus 1 should appear in less than a minute. When it appears, select **Connect**.

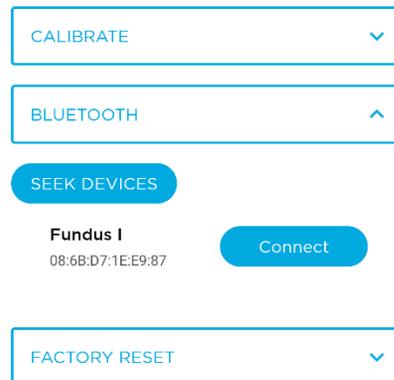

If you need any additional assistance, please contact customer support at support@volk.com, or call us at 440-942-6161.